



US008569052B2

(12) **United States Patent**
Federspiel et al.

(10) **Patent No.:** **US 8,569,052 B2**
(45) **Date of Patent:** **Oct. 29, 2013**

(54) **OXYGEN DEPLETION DEVICES AND METHODS FOR REMOVING OXYGEN FROM RED BLOOD CELLS**

(75) Inventors: **William J. Federspiel**, Pittsburgh, PA (US); **Brian J. Frankowski**, Imperial, PA (US); **Tatsuro Yoshida**, West Newton, MA (US); **Paul J. Vernucci**, Billerica, MA (US)

(73) Assignees: **New Health Sciences, Inc.**, Bethesda, MD (US); **University of Pittsburgh-Of the Commonwealth System of Higher Education**, Pittsburgh, PA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **13/115,532**

(22) Filed: **May 25, 2011**

(65) **Prior Publication Data**

US 2012/0100523 A1 Apr. 26, 2012

Related U.S. Application Data

(63) Continuation of application No. 12/903,057, filed on Oct. 12, 2010, now abandoned.

(60) Provisional application No. 61/250,661, filed on Oct. 12, 2009.

(51) **Int. Cl.**
C12N 5/00 (2006.01)

(52) **U.S. Cl.**
USPC **435/325; 435/283.1**

(58) **Field of Classification Search**
USPC 435/2, 325, 283.1
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,086,924 A	5/1978	Latham, Jr.	
4,228,032 A	10/1980	Talcott	252/400 R
4,300,559 A	11/1981	Gajewski et al.	128/272
4,370,160 A	1/1983	Ziemelis	
4,381,775 A	5/1983	Nose' et al.	
4,540,416 A	9/1985	Hattori et al.	
4,572,899 A	2/1986	Walker et al.	
4,585,735 A	4/1986	Meryman et al.	
4,654,053 A	3/1987	Sievers et al.	
4,670,013 A	6/1987	Barnes et al.	
4,701,267 A	10/1987	Watanabe et al.	
4,713,176 A	12/1987	Schoendorfer et al.	
4,748,121 A	5/1988	Beaver et al.	
4,749,551 A	6/1988	Borgione	422/48
4,769,175 A	9/1988	Inoue	
4,769,318 A	9/1988	Hamasaki et al.	

4,837,047 A	6/1989	Sato et al.	
4,880,548 A	11/1989	Pall et al.	
4,880,786 A	11/1989	Sasakawa et al.	
4,902,701 A	2/1990	Batchelor et al.	
4,925,572 A	5/1990	Pall	
5,000,848 A	3/1991	Hodgins et al.	
5,023,054 A	6/1991	Sato et al.	
5,037,419 A	8/1991	Valentine et al.	
5,152,905 A	10/1992	Pall et al.	
5,192,320 A	3/1993	Anazawa et al.	623/12
5,208,335 A	5/1993	Ramprasad et al.	
5,229,012 A	7/1993	Pall et al.	
5,254,248 A	10/1993	Nakamura et al.	
5,353,793 A	10/1994	Bornn	
5,356,375 A	10/1994	Higley	
5,362,442 A	11/1994	Kent	
5,386,014 A	1/1995	Nho et al.	
5,387,624 A	2/1995	Morita et al.	
5,417,986 A	5/1995	Reid et al.	
5,427,663 A	6/1995	Austin et al.	
5,443,743 A	8/1995	Gsell	
5,476,764 A	12/1995	Bitsensky	
5,506,141 A	4/1996	Weinreb et al.	
5,529,821 A	6/1996	Ishikawa et al.	
5,617,873 A	4/1997	Yost et al.	
5,624,794 A	4/1997	Bitsensky et al.	435/2
5,635,358 A	6/1997	Wilding et al.	
5,691,452 A	11/1997	Gawryl et al.	
5,693,230 A	12/1997	Asher	
5,698,250 A	12/1997	DelDuca et al.	
5,730,989 A	3/1998	Wright	
5,750,115 A	5/1998	Van Den Bosch	
5,783,094 A	7/1998	Kraus et al.	
5,783,148 A	7/1998	Cottingham et al.	

(Continued)

FOREIGN PATENT DOCUMENTS

DE	3722984	1/1989
EP	0 100 419 A2	2/1984

(Continued)

OTHER PUBLICATIONS

International Search Report and Written Opinion dated Apr. 27, 2011 for corresponding International Patent Application No. PCT/US2010/044045.

(Continued)

Primary Examiner — Ruth Davis
(74) *Attorney, Agent, or Firm* — Arnold & Porter LLP

(57) **ABSTRACT**

An oxygen depletion device. The device has a cartridge; a plurality of hollow fibers extending within the cartridge from an entrance to an exit thereof; an amount of an oxygen scavenger packed within the cartridge and contiguous to and in between the plurality of hollow fibers. The hollow fibers are adapted to receiving and conveying red blood cells. There is another embodiment of an oxygen depletion device and method for removing oxygen from red blood cells.

17 Claims, 5 Drawing Sheets

(56)

References Cited

U.S. PATENT DOCUMENTS

5,789,151 A 8/1998 Bitensky et al.
 5,811,142 A 9/1998 DelDuca et al.
 5,846,427 A 12/1998 Kessler et al.
 5,972,710 A 10/1999 Weigl et al.
 6,027,623 A 2/2000 Ohkawa
 6,047,203 A 4/2000 Sackner et al.
 6,090,062 A 7/2000 Sood et al.
 6,150,085 A 11/2000 Hess et al.
 6,162,396 A 12/2000 Bitensky et al. 422/44
 6,187,572 B1 2/2001 Platz et al.
 6,210,601 B1 4/2001 Hottle et al.
 6,231,770 B1 5/2001 Bormann et al.
 6,254,628 B1 7/2001 Wallace et al.
 6,337,026 B1 1/2002 Lee et al.
 6,368,871 B1 4/2002 Christel et al.
 6,387,461 B1 5/2002 Ebner et al.
 6,403,124 B1 6/2002 Dottori
 6,413,713 B1 7/2002 Serebrennikov
 6,439,577 B2 8/2002 Jorgensen et al.
 6,447,987 B1 9/2002 Hess et al.
 6,468,732 B1 10/2002 Malin et al. 435/2
 6,475,147 B1 11/2002 Yost et al.
 6,482,585 B2 11/2002 Dottori
 6,527,957 B1 3/2003 Deniega et al.
 6,564,207 B1 5/2003 Abdoh
 6,610,772 B1 8/2003 Clauberg et al.
 6,688,476 B2 2/2004 Breillatt, Jr. et al.
 6,695,803 B1 2/2004 Robinson et al.
 6,697,667 B1 2/2004 Lee et al.
 6,723,051 B2 4/2004 Davidson et al.
 6,761,695 B2 7/2004 Yost et al.
 6,773,407 B2 8/2004 Yost et al.
 6,817,979 B2 11/2004 Nihtilä
 6,866,783 B2* 3/2005 Baurmeister et al. 210/649
 6,955,648 B2 10/2005 Mozayeni et al.
 7,104,958 B2 9/2006 Crutchfield et al.
 7,208,120 B2 4/2007 Bitensky et al.
 7,347,887 B2 3/2008 Bulow et al.
 7,361,277 B2 4/2008 Bormann et al.
 7,431,995 B2 10/2008 Smith et al.
 7,452,601 B2 11/2008 Ebner et al.
 7,721,898 B2 5/2010 Yagi et al.
 7,723,017 B2 5/2010 Bitensky et al.
 7,754,798 B2 7/2010 Ebner et al.
 7,775,376 B2 8/2010 Bonaguidi et al.
 8,071,282 B2 12/2011 Bitensky et al.
 2001/0027156 A1 10/2001 Egozy et al.
 2002/0062078 A1 5/2002 Crutchfield et al.
 2002/0066699 A1 6/2002 Boggs et al.
 2002/0085952 A1 7/2002 Ellingboe et al.
 2002/0086329 A1 7/2002 Shvets et al.
 2002/0099570 A1 7/2002 Knight
 2002/0182241 A1 12/2002 Borenstein et al.
 2003/0003575 A1 1/2003 Vacanti et al.
 2003/0062299 A1 4/2003 Lee et al.
 2003/0124504 A1 7/2003 Bitensky et al.
 2003/0183801 A1 10/2003 Yang et al.
 2003/0189003 A1 10/2003 Kraus et al.
 2004/0026341 A1 2/2004 Hogberg et al.
 2004/0168982 A1 9/2004 Bitensky et al.
 2005/0038342 A1 2/2005 Mozayeni et al.
 2005/0137517 A1 6/2005 Blickhan et al.
 2005/0139806 A1 6/2005 Havens et al.
 2005/0208462 A1 9/2005 Bitensky et al.
 2005/0230856 A1 10/2005 Parekh et al. 261/122.1
 2005/0233302 A1 10/2005 Hess et al.
 2006/0081524 A1 4/2006 Sengupta et al.
 2006/0118479 A1 6/2006 Shevkoplyas et al.
 2007/0078113 A1 4/2007 Roth et al.
 2007/0240569 A1 10/2007 Ooya
 2008/0243045 A1 10/2008 Pasqualini 604/5.04
 2009/0017128 A1 1/2009 Monzyk et al.
 2009/0269837 A1 10/2009 Shevkoplyas et al.
 2010/0221697 A1 9/2010 Sehgal
 2010/0313755 A1 12/2010 Koros et al.

2012/0024156 A1 2/2012 Yoshida et al.
 2012/0129148 A1 5/2012 Hess et al.
 2012/0219633 A1 8/2012 Sowemimo-Coker

FOREIGN PATENT DOCUMENTS

EP 0 217 759 A1 4/1987
 EP 0 299 381 A2 1/1989
 EP 0 890 368 A1 1/1999
 FR 2 581 289 A1 11/1986
 GB 1 044 649 A2 10/1966
 JP 58-194879 11/1983
 JP 63-63616 A 3/1988
 JP 01-104271 A 4/1989
 JP 5-503075 A 5/1993
 JP 5-503304 A 6/1993
 JP 5-305123 A 11/1993
 JP 06-121920 A 5/1994
 JP 2700170 B2 1/1998
 JP 2000-516963 A 12/2000
 JP 2002-253936 A 9/2002
 JP 2005-535279 A 11/2005
 KR 10-0721054 5/2006
 SU 1718766 A1 1/1990
 WO WO 81/02239 A1 8/1981
 WO WO 86/00809 A1 2/1986
 WO WO 89/02274 A1 3/1989
 WO WO 91/04659 A1 4/1991
 WO WO 92/08348 A1 5/1992
 WO WO 95/29662 A2 11/1995
 WO WO 96/29864 A1 10/1996
 WO WO 99/48963 A2 9/1999
 WO WO 03/043571 A2 5/2003
 WO WO 2006-057473 A1 6/2006
 WO WO 2006/057473 A1 6/2006
 WO WO 2011/014855 A2 2/2011

OTHER PUBLICATIONS

International Search Report and Written Opinion dated Feb. 18, 2011 for corresponding International Patent Application No. PCT/US2010/052084.
 International Search Report and Written Opinion dated Dec. 6, 2010 for corresponding International Patent Application No. PCT/US2010/052376.
 International Preliminary Report on Patentability Dated May 24, 2012 From Corresponding PCT Application No. PCT/US2010/52376.
 Alcantar et al., "Polyethylene glycol-coated biocompatible surfaces," *Journal of Biomedical Materials Research*, 51(3):343-351 (2000).
 Anderson et al., "Microfabrication and microfluidics for tissue engineering: state of the art and future opportunities," *Lab Chip*, 4:98-103 (2004).
 Barbee et al., "The Fahraeus Effect," *Microvascular Research*, 3:6-16 (1971).
 Barclay et al., "A Method for Detecting Chaos in Canine Myocardial Microcirculatory Red Cell Flux," *Microcirculation*, 7(5):335-346 (2000).
 Bardy et al., "Technetium-99m Labeling by Means of Stannous Pyrophosphate: Application to Bleomycin and Red Blood Cells," *Journal of Nuclear Medicine*, 16(5):435-437 (1975).
 Barras et al., "Einfluss der Rejuvenation auf die rheologischen Eigenschaften gelagerter Erythrozyten," *VASA*, 23(4):305-311 (1994).
 Beutler et al., "Storage of red cell concentrates in CPD-A2 for 42 and 49 days," *The Journal of Laboratory and Clinical Medicine*, 102(1):53-62 (1983).
 Borenstein et al., "Microfabrication Technology for Vascularized Tissue Engineering," *Biomedical Microdevices*, 4(3):167-175 (2002).
 Brody et al., "Deformation and Flow of Red Blood Cells in a Synthetic Lattice: Evidence for an Active Cytoskeleton," *Biophysical Journal*, 68:2224-2232 (1995).
 Carmen, "The Selection of Plastic Materials for Blood Bags," *Transfusion Medicine Reviews*, 7(1):1-10 (1993).

(56)

References Cited

OTHER PUBLICATIONS

- Carr et al., "Nonlinear Dynamics of Microvascular Blood Flow," *Annals of Biomedical Engineering*, 28:641-652 (2000).
- Cell Deformability, RheoSCAN (RheoScan-AnD300/RheoScan-D300), obtained on Dec. 11, 2012, from: <http://www.rheoscan.com/products/products/products-01.html>.
- Chilton et al., "Privacy Protection of Health Information: Patient Rights and Pediatrician Responsibilities," *Pediatrics*, 104(4):973-977 (1999).
- Cokelet et al., "Fabrication of in Vitro Microvascular Blood Flow Systems by Photolithography," *Microvascular Research*, 46:394-400 (1993).
- Dale et al., "Human Vaccination with *Escherichia coli* J5 Mutant Induces Cross-Reactive Bactericidal Antibody against *Neisseria gonorrhoeae* Lipooligosaccharide," *The Journal of Infectious Diseases*, 166:316-325 (1992).
- De Angelis et al., "Erythrocyte Shape Control in Stored Blood: The Effect of Additive Solutions on Shape Recovery," *Haematologica*, 73:7-12 (1988).
- Deible et al., "Molecular barriers to biomaterial thrombosis by modification of surface proteins with polyethylene glycol," *Biomaterials*, 19:1885-1893 (1998).
- De Venuto et al., "Rejuvenation of Human Red Blood Cells During Liquid Storage," *Transfusion*, 14(4):338-344 (1974).
- Dumaswala et al., "Studies in Red Blood Cell Preservation: 9. The Role of Glutamine in Red Cell Preservation," *Vox Sang.*, 67:255-259 (1994).
- Dumaswala et al., "Glutamine- and Phosphate-Containing Hypotonic Storage Media Better Maintain Erythrocyte Membrane Physical Properties," *Blood*, 88(2):697-704 (1996).
- Dumaswala et al., "Improved Red Blood Cell Preservation Correlates With Decreased Loss of Bands 3, 4.1, Acetylcholinesterase, and Lipids in Microvesicles," *Blood*, 87(4):1612-1616 (1996).
- Dumont et al., "Anaerobic storage of red blood cells in a novel additive solution improves in vivo recovery," *Transfusion*, 49(3):458-464 (2009).
- Effenhauser et al., "Integrated Capillary Electrophoresis on Flexible Silicone Microdevices: Analysis of DNA Restriction Fragments and Detection of Single DNA Molecules on Microchips," *Anal. Chem.*, 69:3451-3457 (1997).
- European Search Report completed on Feb. 11, 2005, in European Patent Application No. 02 78 2307.9.
- Fahraeus et al., "The Viscosity of the Blood in Narrow Capillary Tubes," *Am. J. Physiol.*, 96(3):562-568 (1931).
- Fang et al., "Inhibition of Lipopolysaccharide-Associated Endotoxin Activities In Vitro and In Vivo by the Human Anti-Lipid A Monoclonal Antibody SdJ5-1.17.15," *Infection and Immunity*, 61(9):3873-3878 (1993).
- Frame et al., "A System for Culture of Endothelial Cells in 20-50- μ m Branching Tubes," *Microcirculation*, 2 (4):377-385 (1995).
- Fung et al., "High-Resolution Data on the Geometry of Red Blood Cells," *Biorheology*, 18:369-385 (1981).
- Gañán-Calvo et al., "Current and Droplet Size in the Electro spraying of Liquids. Scaling Laws," *J. Aerosol Sci.*, 28(2):249-275 (1997).
- Green et al., "10. Liposomal Vaccines," *Immunobiology of Proteins and Peptides VII*, Plenum Press, New York, pp. 83-92 (1995).
- Greenwalt et al., "Studies in Red Blood Cell Preservation. 7. In vivo and in Vitro Studies with a Modified Phosphate-Ammonium Additive Solution," *Vox Sang.*, 65:87-94 (1993).
- Greenwalt et al., "Studies in Red Blood Cell Preservation. 8. Liquid Storage of Red Cells in Glycerol-Containing Additive Solution," *Vox Sang.*, 67:139-143 (1994).
- Greenwalt et al., "Studies in red blood cell preservation. 10. ⁵¹Cr Recovery of Red Cells after Liquid Storage in a Glycerol-Containing Additive Solution," *Vox Sang.*, 70:6-10 (1996).
- Greenwalt et al., "The effect of hypotonicity, glutamine, and glycine on red cell preservation," *Transfusion*, 37:269-276 (1997).
- Griffith, "Temporal chaos in the microcirculation," *Cardiovascular Research*, 31:342-358 (1996).
- Hamasaki et al., "Acid-citrate-dextrose-phosphoenolpyruvate medium as a rejuvenant for blood storage," *Transfusion*, 23(1):1-7 (1983).
- Hess, "Extended Liquid Storage of Red Blood Cells," *Blood Donors and the Supply of Blood and Blood Products*, National Academy Press, Washington, D.C., pp. 99-102 (1996).
- Hess et al., "Successful storage of RBCs for 9 weeks in a new additive solution," *Transfusion*, 40:1007-1011 (2000).
- Hess, "Storage of red blood cells under anaerobic conditions," *Vox Sanguinis*, 93:183 (2007).
- Hodgson et al., "Prophylactic use of human endotoxin-core hyperimmune gammaglobulin to prevent endotoxaemia in colostrum-deprived, gnotobiotic lambs challenged orally with *Escherichia coli*," *FEMS Immunology and Medical Microbiology*, 11:171-180 (1995).
- Högman et al., "Cell Shape and Total Adenylate Concentration as Important Factors for Posttransfusion Survival of Erythrocytes," *Biomed. Biochim. Acta*, 42:S327-S331 (1983).
- Högman et al., "Effects of Oxygen on Red Cells during Liquid Storage at +4° C," *Vox Sang.*, 51:27-34 (1986).
- Högman et al., "Effects of Oxygen and Mixing on red cells stored in plastic bags at +4° C," *Biomed. Biochim. Acta.*, 46:S290-S294 (1987).
- Högman et al., "Shall Red Cell Units Stand Upright, Lie Flat or be Mixed During Storage? In Vitro Studies of Red Cells Collected in 0.5 CPD and Stored in RAS2 (Erythrosol®)," *Transfus. Sci.*, 16(2):193-199 (1995).
- Huang et al., "Continuous Particle Separation Through Deterministic Lateral Displacement," *Science*, 304:987-990 (2004).
- International Preliminary Report on Patentability completed on Feb. 14, 2012, in International Patent Application No. PCT/US2010/52084.
- International Preliminary Report on Patentability completed on May 21, 2012, in International Patent Application No. PCT/US2010/52376.
- International Preliminary Report on Patentability completed on Oct. 18, 2011, in International Patent Application No. PCT/US2010/031055.
- International Search Report completed on Jul. 8, 1996, in International Patent Application No. PCT/US96/09005.
- International Search Report completed on Nov. 10, 2003, in International Patent Application No. PCT/US02/36735.
- International Search Report completed on May 20, 2010, in International Patent Application No. PCT/US2010/31055.
- International Search Report completed on Apr. 26, 2011, in International Patent Application No. PCT/US2010/044045.
- International Search Report completed on Dec. 21, 2011, in International Patent Application No. PCT/US11/49168.
- International Search Report completed on Feb. 12, 2012, in International Patent Application No. PCT/US11/59372.
- International Search Report completed on Jun. 18, 2012, in International Patent Application No. PCT/US12/30930.
- International Search Report completed on Sep. 24, 2012, in International Patent Application No. PCT/US12/50380.
- Jain, et al., "Determinants of Leukocyte Margination in Rectangular Microchannels," *PLoS ONE*, 4(9):1-8 (2009).
- Jayasinghe et al., "Controlled deposition of nanoparticle clusters by electrohydrodynamic atomization," *Nanotechnology*, 15:1519-1523 (2004).
- Jiang et al., "Microfluidic synthesis of monodisperse PDMS microbeads as discrete oxygen sensors," *Soft Matter*, 8:923-926 (2011).
- Jo et al., "Surface modification using silanated poly(ethylene glycol)s," *Biomaterials*, 21:605-616 (2000).
- Johnson et al., "Regulation of blood flow in single capillaries," *American Journal of Physiology*, 212:1405-1415 (1967).
- Kaihara et al., "Silicon Micromachining to Tissue Engineer Branched Vascular Channels for Liver Fabrication," *Tissue Engineering*, 6(2):105-117 (2000).
- Kiani et al., "Fluctuations in microvascular blood flow parameters caused by hemodynamic mechanisms," *American Journal of Physiology*, 266(5):H1822-H1828 (1994).

(56)

References Cited

OTHER PUBLICATIONS

- Kikuchi et al., "Modified Cell-Flow Microchannels in a Single-Crystal Silicon Substrate and Flow Behavior of Blood Cells," *Microvascular Research*, 47:126-139 (1994).
- Koch et al., "Peripheral blood leukocyte NO production and oxidative stress in multiple sclerosis," *Multiple Sclerosis*, 14:159-165 (2008).
- Koch et al., "Duration of Red-Cell Storage and Complications After Cardiac Surgery," *The New England Journal of Medicine*, 358:1229-1239 (2008).
- Krogh, "Studies on the physiology of capillaries. II. The reactions to local stimuli of the blood-vessels in the skin and web of the frog," *The Journal of Physiology*, 55:412-422 (1921).
- Kuraoka, et al., "Ship-in-a-bottle synthesis of a cobalt phthalocyanine/porous glass composite membrane for oxygen separation," *Journal of Membrane Science*, 286(1-2):12-14 (2006).
- Lugowski et al., "Anti-endotoxin antibodies directed against *Escherichia coli* R-1 oligosaccharide core-tetanus toxoid conjugate bind to smooth, live bacteria and smooth lipopolysaccharides and attenuate their tumor necrosis factor stimulating activity," *FEMS Immunology and Medical Microbiology*, 16:31-38 (1996).
- Mazor et al., "Prolonged Storage of Red Cells: The Effect of pH, Adenine Phosphate," *Vox Sanguinis*, 66:264-269 (1994).
- McDonald et al., "Poly(dimethylsiloxane) as a Material for Fabricating Microfluidic Devices," *Accounts of Chemical Research*, 35(7):491-499 (2002).
- Meryman et al., "Prolonged storage of red cells at 4° C," *Transfusion*, 26(6):500-505 (1986).
- Meryman et al., "Extending the storage of red cells at 4° C," *Transfus. Sci.*, 15(2):105-115 (1994).
- Moll et al., "Dean vortices applied to membrane process. Part II: Numerical approach," *Journal of Membrane Science*, 288:321-335 (2007).
- Moroff et al., "Proposed standardization of methods for determining the 24-hour survival of stored red cells," *Transfusion*, 24:109-114 (1984).
- Murphy et al., "Increased Mortality, Postoperative Morbidity, and Cost After Red Blood Cell Transfusion in Patients Having Cardiac Surgery," *Circulation*, 116:2544-2552 (2007).
- Ng et al., "Components for integrated poly(dimethylsiloxane) microfluidic systems," *Electrophoresis*, 23:3461-3473 (2002).
- Ohkuma et al., "The preservative-exchange method using a sextuple-bag system for a 10-week storage period of red blood cells," *Transfusion Medicine*, 1:257-262 (1991).
- Poxton, "Antibodies to lipopolysaccharide," *Journal of Immunological Methods*, 186:1-15 (1995).
- Pries et al., "Biophysical aspects of blood flow in the microvasculature," *Cardiovascular Research*, 32:654-667 (1996).
- Sambuceti et al., "Why should we study the coronary microcirculation?," *Am J Physiol Heart Circ Physiol*, 279:H2581-H2584 (2000).
- Shevkopyas et al., "Direct measurement of the impact of impaired erythrocyte deformability on microvascular network perfusion in a microfluidic device," *Lab Chip*, 6:914-920 (2006).
- Shimizu et al., "Multicenter Clinical Evaluation of Red Cell Concentrates Stored up to 6 Weeks in MAP, a new additive solution," *Japanese Journal of Clinical Hematology*, 33(2):148-156 (1992).
- Skalak et al., "Deformation of Red Blood Cell in Capillaries," *Science*, 164(3880):717-719 (1969).
- Sohmer et al., "Phosphoenolpyruvate (PEP) Effects on Fresh and Stored Red Blood Cells," *Proceedings of the Society for Experimental Biology and Medicine*, 171:24-33 (1982).
- Sutton et al., "A Novel Instrument for Studying the Flow Behaviour of Erythrocytes through Microchannels Simulating Human Blood Capillaries," *Microvascular Research*, 53:272-281 (1997).
- Szymanski et al., "Effect of rejuvenation and frozen storage on 42-day-old AS-1 RBCs," *Transfusion*, 41:550-555 (2001).
- The International Committee for Standardization in Hematology, "Recommended Methods for Radioisotope Red Cell Survival Studies," *Blood*, 38(3):378-386 (1971).
- Tinmouth et al., "The Clinical Consequences of the Red Cell Storage Lesion," *Transfusion Medicine Reviews*, 15(2):91-107 (2001).
- Tracey et al., "A Silicon Micromachined Device for Use in Blood Cell Deformability Studies," *IEEE Transactions on Biomedical Engineering*, 42(8):751-761 (1995).
- Tsukada et al., "Direct Measurement of Erythrocyte Deformability in Diabetes Mellitus with a Transparent Microchannel Capillary Model and High-Speed Video Camera System," *Microvascular Research*, 61:231-239 (2001).
- Valeri et al., "The survival, function, and hemolysis of human RBCs stored at 4° C in additive solution (AS-1, AS-3, or AS-5) for 42 days and then biochemically modified, frozen, thawed, washed, and stored at 4° C in sodium chloride and glucose solution for 24 hours," *Transfusion*, 40:1341-1345 (2000).
- Wang et al., "Fabrication of PLGA microvessel scaffolds with circular microchannels using soft lithography," *Journal of Micromechanics and Microengineering*, 17(10):2000-2005 (2007).
- Weinberg et al., "Transfusions in the Less Severely injured: Does Age of Transfused Blood Affect Outcomes?," *The Journal of Trauma*, 65(4):794-798 (2008).
- Wilding et al., "Manipulation and Flow of Biological Fluids in Straight Channels Micromachined in Silicon," *Clinical Chemistry*, 40(1):43-47 (1994).
- Wood et al., "The Viability of Human Blood Stored in Phosphate Adenine Media," *Transfusion*, 7(6):401-408 (1967).
- Wu et al., "Polymer microchips bonded by O₂-plasma activation," *Electrophoresis*, 23:782-790 (2002).
- Yoshida et al., "Extended storage of red blood cells under anaerobic conditions," *Vox Sanguinis*, 92:22-31 (2007).
- Yoshida et al., "Storage of red blood cells under anaerobic conditions: reply," *Vox Sanguinis*, 93:184 (2007).
- Yoshida et al., "The effects of additive solution pH and metabolic rejuvenation on anaerobic storage of red cells," *Transfusion*, 48:2096-2105 (2008).
- Yoshida et al., "Anaerobic storage of red blood cells," *Blood Transfus*, 8:220-236 (2010).
- Zhang et al., "Modification of Si(100) surface by the grafting of poly(ethylene glycol) for reduction in protein adsorption and platelet adhesion," *J Biomed Mater Res*, 56:324-332 (2001).
- Zimrin et al., "Current issues relating to the transfusion of stored red blood cells," *Vox Sanguinis*, 96:93-103 (2009).

* cited by examiner

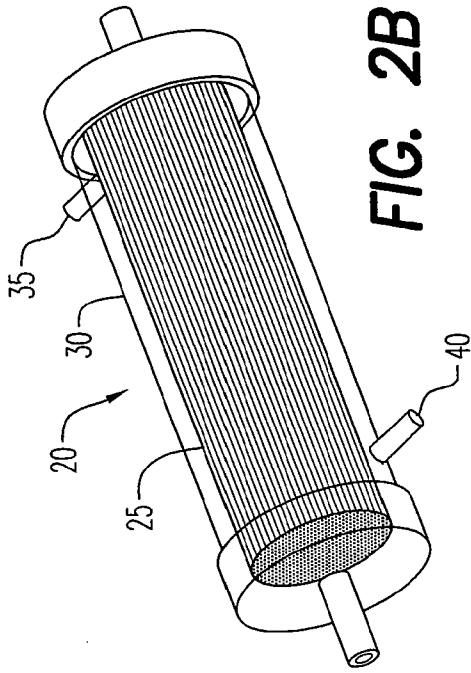


FIG. 2A

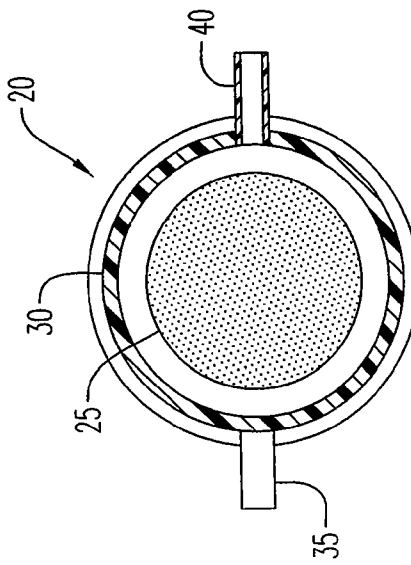


FIG. 2B

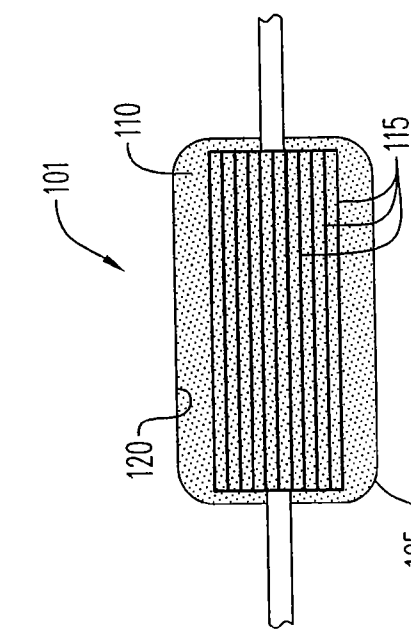


FIG. 2C

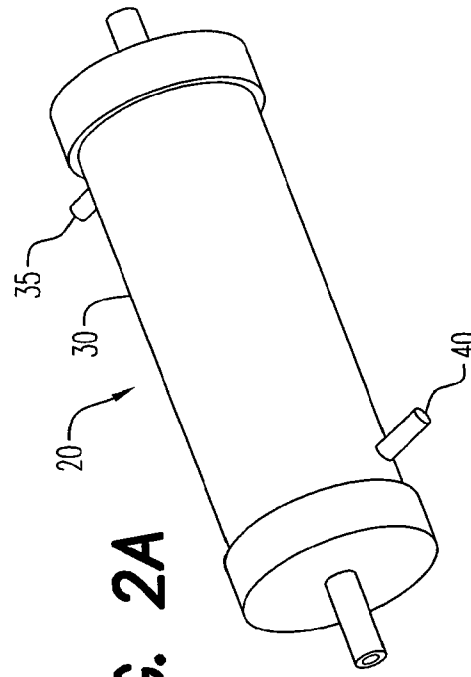


FIG. 1

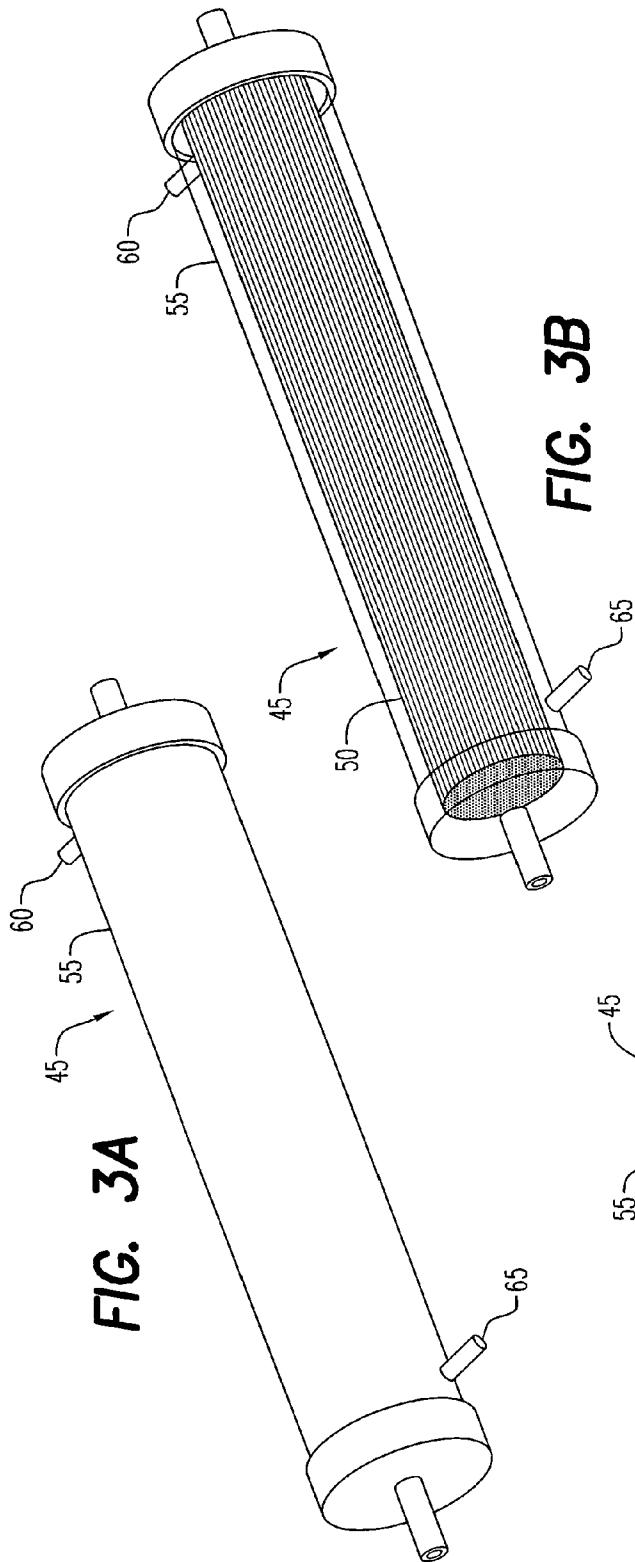


FIG. 3B

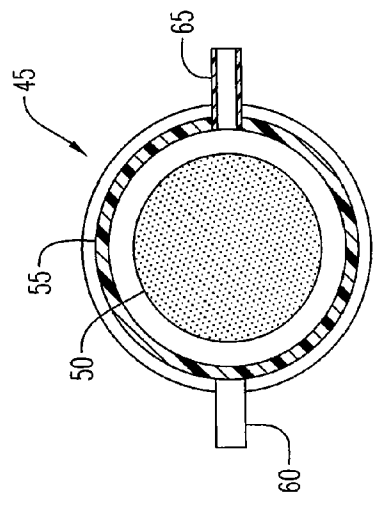


FIG. 3C

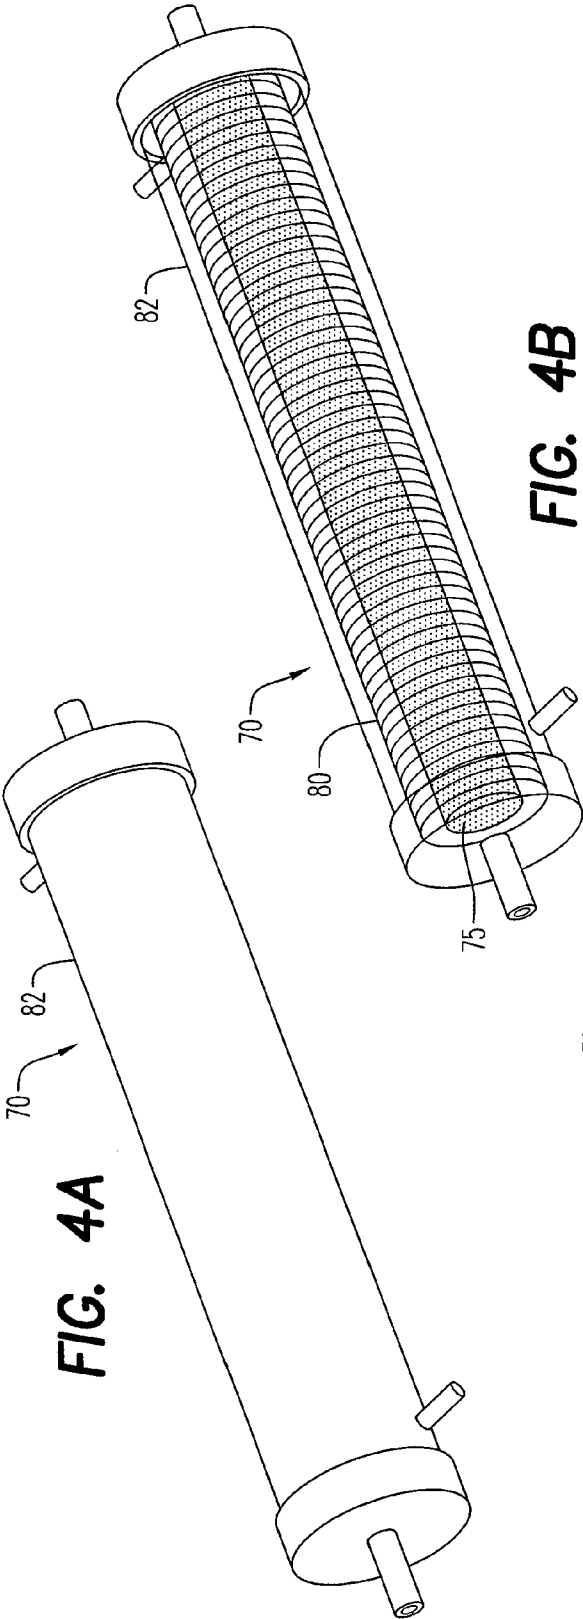


FIG. 4B

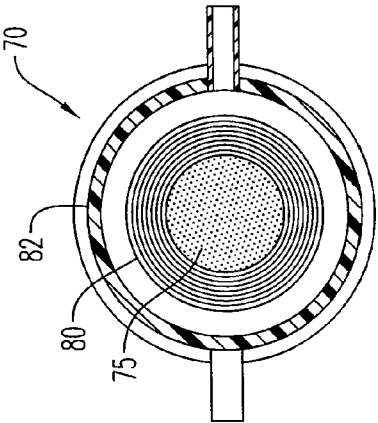


FIG. 4C

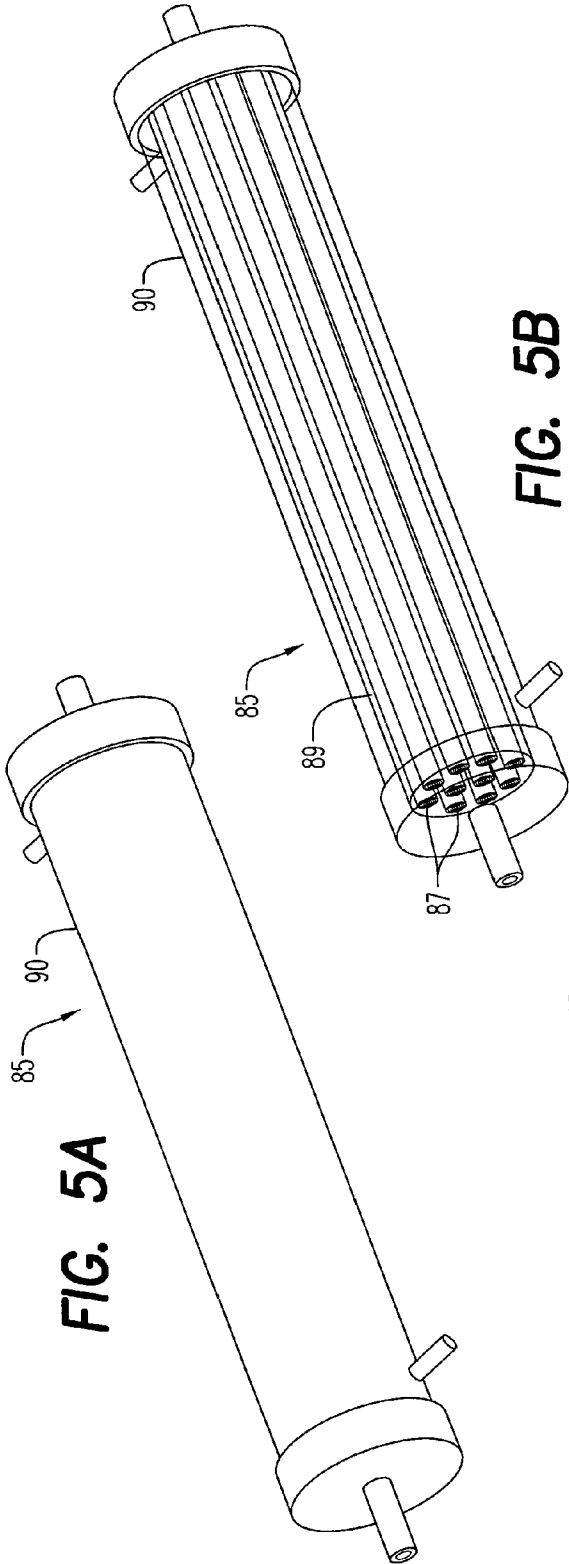


FIG. 5B

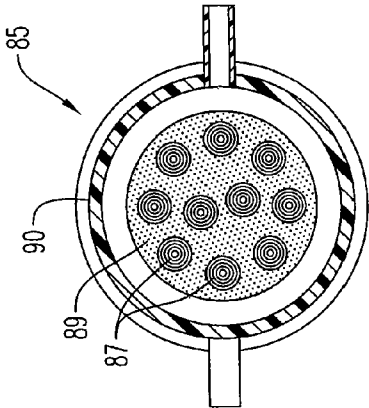


FIG. 5C

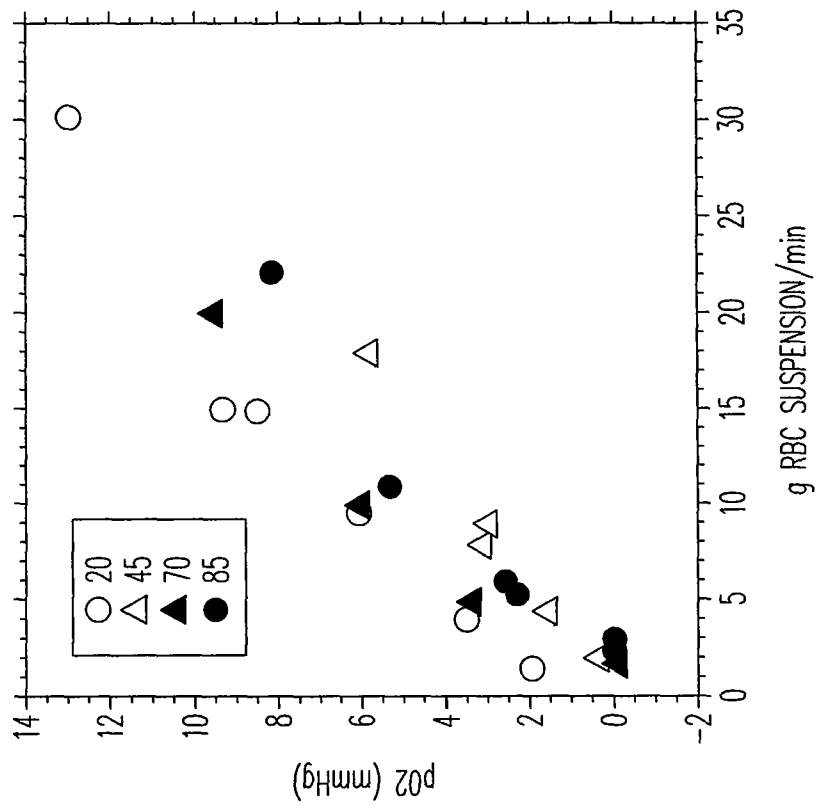


FIG. 6

OXYGEN DEPLETION DEVICES AND METHODS FOR REMOVING OXYGEN FROM RED BLOOD CELLS

CROSS-REFERENCE TO RELATED APPLICATIONS

The present application is a Continuation application of U.S. patent application Ser. No. 12/903,057, filed on Oct. 12, 2010 now abandoned, which claims priority based on U.S. Provisional Application No. 61/250,661, filed Oct. 12, 2009, both of which are incorporated herein by reference in its entirety.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH

This invention was made with government support under grants awarded by the National Institutes of Health (NIH) and the National Heart Lung and Blood Institute (NHLBI). The government has certain rights in the invention.

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention relates to devices for depleting oxygen from red blood cells to enhance storage life. The present invention relates to methods for depleting oxygen from red blood cells.

2. Background of the Art

Adequate blood supply and the storage thereof is a problem facing every major hospital and health organization around the world. Often, the amount of blood supply in storage is considerably smaller than the need therefor. This is especially true during crisis periods such as natural catastrophes, war and the like, when the blood supply is often perilously close to running out. It is at critical times such as these that the cry for more donations of fresh blood is often heard. However, unfortunately, even when there is no crisis period, the blood supply and that kept in storage must be constantly monitored and replenished, because stored blood does not maintain its viability for long.

Stored blood undergoes steady deterioration which is, in part, caused by hemoglobin oxidation and degradation and adenosine triphosphate (ATP) and 2-3-biphosphoglycerate (DPG) depletion. Oxygen causes hemoglobin (Hb) carried by the red blood cells (RBCs) to convert to met-Hb, the breakdown of which produces toxic products such as hemichrome, hemin and free Fe^{3+} . Together with the oxygen, these products catalyze the formation of hydroxyl radicals (OH \cdot), and both the OH \cdot and the met-Hb breakdown products damage the red blood cell lipid membrane, the membrane skeleton, and the cell contents. As such, stored blood is considered unusable after 6 weeks, as determined by the relative inability of the red blood cells to survive in the circulation of the transfusion recipient. The depletion of DPG prevents adequate transport of oxygen to tissue thereby lowering the efficacy of transfusion immediately after administration (levels of DPG recover once in recipient after 8-48 hrs). In addition, these deleterious effects also result in reduced overall efficacy and increased side effects of transfusion therapy with stored blood before expiration date, but possibly older than two weeks are used.

There is, therefore, a need to be able to deplete oxygen levels in red blood cells prior to storage on a long-term basis

without the stored blood undergoing the harmful effects caused by the oxygen and hemoglobin interaction.

SUMMARY OF THE INVENTION

Accordingly, the present disclosure provides for a disposable device that is able to remove oxygen from red blood cells.

The present disclosure provides for an oxygen depletion device. The device has a cartridge; a plurality of hollow fibers extending within the cartridge from an entrance to an exit thereof; an amount of an oxygen scavenger packed within the cartridge and contiguous to and in between the plurality of hollow fibers. The hollow fibers are adapted to receiving and conveying red blood cells.

The present disclosure provides for an oxygen depletion device. The device has a receptacle of a solid material having an inlet and an outlet adapted to receiving and expelling a flushing gas and a plurality of hollow fibers extending within the receptacle from an entrance to an exit thereof. The hollow fibers are adapted to receiving and conveying red blood cells.

The present disclosure provides for a method for removing oxygen from red blood cells. The method has the step of passing the red blood cells through an oxygen device. The device has a cartridge; a plurality of hollow fibers extending within the cartridge from an entrance to an exit thereof; and an amount of an oxygen scavenger packed within the cartridge and contiguous to and in between the plurality of hollow fibers. The hollow fibers are adapted to receiving and conveying red blood cells.

The present disclosure provides for a method for removing oxygen from red blood cells. The method has the step of passing the red blood cells through an oxygen device. The device has a receptacle of a solid material having an inlet and an outlet adapted to receiving and expelling a flushing gas; and a plurality of hollow fibers films extending within the receptacle from an entrance to an exit thereof. The hollow fibers are adapted to receiving and conveying red blood cells.

The present disclosure and its features and advantages will become more apparent from the following detailed description with reference to the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a pre-storage oxygen depletion device of the present invention.

FIG. 2a illustrates an embodiment of a depletion device that depletes oxygen from red blood cells prior to storage by a flushing inert gas around a hollow fiber inside the assembly.

FIG. 2b illustrates an embodiment of a depletion device that depletes oxygen from red blood cells prior to storage by a flushing inert gas around a hollow fiber inside the assembly.

FIG. 2c illustrates an embodiment of a depletion device that depletes oxygen from red blood cells prior to storage by a flushing inert gas around a hollow fiber inside the assembly.

FIG. 3a illustrates another embodiment of a depletion device that depletes oxygen from red blood cells prior to storage.

FIG. 3b illustrates another embodiment of a depletion device that depletes oxygen from red blood cells prior to storage.

FIG. 3c illustrates another embodiment of a depletion device that depletes oxygen from red blood cells prior to storage.

FIG. 4a illustrates another embodiment of a depletion device that depletes oxygen from red blood cells prior to storage wherein oxygen is scavenged by scavenger materials in the core of the cylinder, surrounded by hollow fibers.

3

FIG. 4b illustrates another embodiment of a depletion device that depletes oxygen from red blood cells prior to storage wherein oxygen is scavenged by scavenger materials in the core of the cylinder, surrounded by hollow fibers.

FIG. 4c illustrates another embodiment of a depletion device that depletes oxygen from red blood cells prior to storage wherein oxygen is scavenged by scavenger materials in the core of the cylinder, surrounded by hollow fibers.

FIG. 5a illustrates another embodiment of a depletion device that depletes oxygen from red blood cells wherein oxygen is scavenged by scavenger materials surrounding cylinders of hollow fibers.

FIG. 5b illustrates another embodiment of a depletion device that depletes oxygen from red blood cells wherein oxygen is scavenged by scavenger materials surrounding cylinders of hollow fibers.

FIG. 5c illustrates another embodiment of a depletion device that depletes oxygen from red blood cells wherein oxygen is scavenged by scavenger materials surrounding cylinders of hollow fibers.

FIG. 6 illustrates a plot of flow rate of RBC suspension per minute versus oxygen partial pressure for the depletion devices of FIGS. 2a through 2c, FIGS. 3a through 3c, FIGS. 4a through 4c and FIGS. 5a through 5c.

DETAILED DESCRIPTION OF THE DISCLOSURE

Referring to FIG. 2, an oxygen depletion device (ODD) 101 contains an oxygen sorbent 110. ODD 101 is a disposable cartridge 105 containing oxygen sorbent 110 and a series of hollow fibers 115. Oxygen sorbent 110 is a mixture of non-toxic inorganic and/or organic salts and ferrous iron or other materials with high reactivity toward oxygen. Oxygen sorbent 110 is made from particles that have significant absorbing capacity for O₂ (more than 5 ml O₂/g) and can maintain the inside of cartridge 105 to less than 0.01%, which corresponds to PO₂ less than 0.08 mmHg. Oxygen sorbent 110 is either free or contained in an oxygen permeable envelope. ODD 101 of the present disclosure can deplete approximately 100 mL of oxygen from a unit of blood.

RBCs pass through hollow porous fibers 115. Porous fibers are capable of high oxygen permeability rates. Suitable materials for porous fibers include polyolefins, TEFLON® (polytetrafluoroethylene), polyesters, polyvinylidene fluoride (PVDF), polysulfone, and other hydrophobic polymers as well as inorganic materials (ceramics). Oxygen depletion takes place as RBCs pass through membrane 115. ODD provides a simple structure having a large surface area to remove oxygen and maintain constant flow of blood therethrough. The oxygen depletion or removal is accomplished by irreversible reaction of ferrous ion in oxygen sorbent 110 with ambient oxygen to form ferric oxide. ODD 101 does not need agitation for oxygen removal and can be manufactured easily to withstand centrifugation as part of a blood collection system as necessary.

Referring to FIGS. 2a through 2c and FIGS. 3a through 3c, examples of flushing depletion devices are disclosed. The depletion devices function to deplete O₂ by supplying appropriate composition of flushing gas. Gases appropriate for depletion devices include, for example, Ar, He, CO₂, N₂.

FIGS. 4a through 4c and 5a through 5c, also disclose scavenging depletion devices. Depletion takes place with the use of scavengers or sorbents and without the use of external gases. In both types of depletion devices however, oxygen depletion is effective to enhance DPG and ATP, respectively, prior to storage in blood storage bags.

4

Referring to FIGS. 2a through 2c, a depletion device 20 is shown. Depletion device 20 includes a plurality of fibers 25, approximately 5000 in number, through which red blood cells flow. Plurality of fibers 25 are surrounded by a plastic cylinder 30. Plastic cylinder 30 contains a gas inlet 35 and a gas outlet 40 through which a flushing gas or a combination of flushing gases, such as those mentioned above, are supplied to remove oxygen from blood. Specifications for depletion device 20 are shown in Table 1 below.

TABLE 1

Prototype Specification	Eternal Gas Pathways	External Gas Pathways
Prototype Serial #:	Device 20	
Fiber Type:	Celgard	Celgard
	200/150-66FPI	200/150-66FPI
Number of Fibers:	5000	5000
Active Length of Fibers (cm):	13	28
Fiber OD (microns):	200	200
Fiber ID (microns):	150	150
Total Length of Fibers:	15	30
Active Fiber Surface Area (m ²):	0.4084	0.8796

Referring to FIGS. 3a through 3c, a depletion device 45 is shown. Depletion device 45, like device 20 of FIGS. 2a to 2c, includes a plurality of fibers 50, approximately 5000 in number, through which red blood cells flow. Plurality of fibers 50 are surrounded by a plastic cylinder 55. Plastic cylinder 55 contains a gas inlet 60 and a gas outlet 65 through which a gas or a combination of gases, such as those mentioned above are supplied to remove oxygen from blood. Specifications for depletion device 45 are shown in Table 2 below. The active surface area of depletion of device 45 is twice that of device 20 because device 45 is twice as long as device 20.

TABLE 2

Prototype Specification	Eternal Gas Pathways	External Gas Pathways
Prototype Serial #:		Device 45
Fiber Type:	Celgard	Celgard
	200/150-66FPI	200/150-66FPI
Number of Fibers:	5000	5000
Active Length of Fibers (cm):	13	28
Fiber OD (microns):	200	200
Fiber ID (microns):	150	150
Total Length of Fibers:	15	30
Active Fiber Surface Area (m ²):	0.4084	0.8796

FIGS. 4a through 4c disclose a depletion device 70 having a core 75 containing scavenging materials for O₂. Core 75 is packed by a gas permeable film with very low liquid permeability. Hollow fibers 80 are wound around core 75, and a plastic cylinder 82 contains and envelopes hollow fibers 80. In this particular embodiment, the active surface area for depletion is approximately 0.8796 m² as shown in Table 3 below.

TABLE 3

Prototype Specification	Center Core 125 grams Sorbent	10 individual Bundles 200 grams Sorbent
Prototype Serial #:	Device 70	
Fiber Type:	Celgard	Celgard
	200/150-66FPI	200/150-66FPI
Number of Fibers:	5000	5000
Active Length of Fibers (cm):	13	28
Fiber OD (microns):	200	200

TABLE 3-continued

Prototype Specification	Center Core 125 grams Sorbent	10 individual Bundles 200 grams Sorbent
Fiber ID (microns):	150	150
Total Length of Fibers	15	30
Active Fiber Surface Area (m ²):	0.8796	0.8796

FIGS. 5a through 5c disclose a depletion device 85 containing fiber bundles 87 enclosed in gas permeable film with very low liquid permeability. Fiber bundles 87 are surrounded by scavenger materials 89 for O₂. Fiber bundles 87 and scavenger materials 89 are contained within a plastic cylinder 90. The active surface area for depletion is approximately 0.8796 m² as shown in Table 4 below.

TABLE 4

Prototype Specification	Center Core 125 grams Sorbent	10 individual Bundles 200 grams Sorbent
Prototype Serial #:		Device 85
Fiber Type:	Celgard	Celgard
	200/150-66FPI	200/150-66FPI
Number of Fibers:	5000	5000
Active Length of Fibers (cm):	13	28
Fiber OD (microns):	200	200
Fiber ID (microns):	150	150
Total Length of Fibers	15	30
Active Fiber Surface Area (m ²):	0.8796	0.8796

FIG. 6 is a plot of the performance of flushing depletion devices 20 and 45 and scavenging depletion devices 70 and 85. The data of FIG. 6 was plotted using the following conditions: Hematocrit, 62% (pooled 3 units of pRBC), and 21° C. at various head heights to produce different flow rates. Oxygen scavenger (Multisorb Technologies, Buffalo, N.Y.) was activated with adding 5% and 12% w/w water vapor for device 79 and device 85, respectively. Data are plotted with flow rate (g RBC suspension per min) vs. pO₂ (mmHg).

In the oxygen depletion devices disclosed herein, the hollow fibers may be packed in any suitable configuration within the cartridge, such as linear or longitudinal, spiral, or coil, so long as they can receive and convey red blood cells.

FIG. 6 shows that lowest oxygen saturation is achieved using devices 45 and 85. Device 45 exhibits a larger active surface area exposed to gases along length of fibers 50. Device 85 also has a long surface area of exposure to scavenging materials. Device 85 has bundles 87 surrounded by scavenging materials 89. The space occupied by scavenging materials 89 between bundles 87 promotes dispersion of oxygen from red blood cells contained in fiber bundles 87, thus aiding scavenging of oxygen from red blood cells.

A further use of the depletion devices is to add back oxygen prior to transfusion by flushing with pure oxygen or air. This use is for special cases, such as massive transfusions, where the capacity of the lung to reoxygenate transfused blood is not adequate, or sickle cell anemia.

Similarly, depletion devices can be used to obtain intermediate levels or states of depletion of oxygen depending needs of the patient to obtain optimal levels in the transfused blood depending upon the patients needs.

It is within the scope of the present invention to remove oxygen from the RBCs or to strip oxygen from the blood prior to storage in the storage bags. An oxygen scavenger can be used to remove the oxygen from the RBCs prior to storage in the blood bags. As used herein, "oxygen scavenger" is a

material that irreversibly binds to or combines with oxygen under the conditions of use. For example, the oxygen can chemically react with some component of the material and be converted into another compound. Any material where the off-rate of bound oxygen is zero can serve as an oxygen scavenger. Examples of oxygen scavengers include iron powders and organic compounds. The term "oxygen sorbent" may be used interchangeably herein with oxygen scavenger. For example, oxygen scavengers are provided by Multisorb Technologies (Buffalo, N.Y.). Such materials can be blended to a desired ratio to achieve desired results.

It will be appreciated that scavengers can be incorporated into storage receptacles and bags in any known form, such as in sachets, patches, coatings, pockets, and packets.

Although the present invention describes in detail certain embodiments, it is understood that variations and modifications exist known to those skilled in the art that are within the invention. Accordingly, the present invention is intended to encompass all such alternatives, modifications and variations that are within the scope of the invention as set forth in the disclosure.

What is claimed is:

1. An oxygen depletion device comprising:

a cartridge;

a plurality of hollow fibers extending within said cartridge from an entrance to an exit thereof, wherein the hollow fibers are formed of an oxygen-permeable membrane and are adapted to receiving and conveying red blood cells; and

an amount of an oxygen scavenger packed within the cartridge and contiguous to and in between the plurality of hollow fibers, wherein said red blood cells are passed within said hollow fibers.

2. The device of claim 1, wherein said hollow fibers are substantially parallel and longitudinally disposed within the cartridge from said entrance to said exit.

3. The oxygen depletion device of claim 1, wherein said oxygen scavenger is ferrous iron.

4. The oxygen depletion device of claim 1, wherein said plurality of hollow fibers are formed from an oxygen-permeable material selected from the group consisting of polyolefin, polytetrafluoroethylene, polyester, polyvinylidene fluoride (PVDF), and polysulfone.

5. The oxygen depletion device of claim 1, wherein said plurality of hollow fibers are formed from a hydrophobic polymer.

6. The oxygen depletion device of claim 1, wherein said plurality of hollow fibers are formed from an inorganic ceramic.

7. The oxygen depletion device of claim 1, wherein said plurality of hollow fibers are configured as a linear spiral, a longitudinal spiral, or a coil.

8. An oxygen depletion device comprising:

a receptacle of a solid material having an inlet and an outlet adapted to receiving and expelling a flushing gas;

a plurality of hollow fibers extending within the receptacle from an entrance to an exit thereof; wherein the hollow fibers are adapted to receiving and conveying red blood cells, wherein said red blood cells are passed within said hollow fibers.

9. The device of claim 8, wherein the hollow fibers are substantially parallel and longitudinally disposed within the cartridge from said entrance to said exit.

10. The device of claim 8, further including a source of flushing gas in communication with said inlet of said receptacle.

7

11. A method for removing oxygen from red blood cells comprising:

passing red blood cells through an oxygen depletion device, wherein the device comprises:

a cartridge;

a plurality of hollow fibers extending within said cartridge from an entrance to an exit thereof, wherein said plurality of hollow fibers are adapted to receiving and conveying red blood cells; and

an amount of an oxygen scavenger packed within said cartridge and contiguous to and in between said plurality of hollow fibers, wherein said red blood cells are passaged within said hollow fibers.

12. The method of claim **11**, wherein said oxygen scavenger is ferrous iron.

13. The method of claim **11**, wherein said plurality of hollow fibers are formed from an oxygen-permeable material selected from the group consisting of polyolefin, polytetrafluoroethylene, polyester, polyvinylidene fluoride (PVDF), and polysulfone.

8

14. The method of claim **11**, wherein said plurality of hollow fibers are formed from a hydrophobic polymer.

15. The method of claim **11**, wherein said plurality of hollow fibers are formed from an inorganic ceramic.

⁵ **16.** The method of claim **11**, wherein said plurality of hollow fibers are configured as a linear spiral, a longitudinal spiral, or a coil.

17. A method for removing oxygen from red blood cells comprising:

passing the red blood cells through an oxygen depletion device, wherein the device comprises:

a receptacle of a solid material having an inlet and an outlet adapted to receiving and expelling a flushing gas;

¹⁰ a plurality of hollow fibers extending within the receptacle from an entrance to an exit thereof, wherein the hollow fibers are adapted to receiving and conveying red blood cells, wherein said red blood cells are passaged within said hollow fibers.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 8,569,052 B2
APPLICATION NO. : 13/115532
DATED : October 29, 2013
INVENTOR(S) : William J. Federspiel et al.

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Claims:

Col. 6, line 43, Claim 4, "polvvinylidene" should read as --polyvinylidene--; and

Col. 7, line 19, Claim 13, "polvvinylidene" should read as --polyvinylidene--.

Signed and Sealed this
Eleventh Day of February, 2014



Michelle K. Lee
Deputy Director of the United States Patent and Trademark Office